



12306 Belton Honea Path Highway, Honea Path, SC 29654
 Ph: (864) 369-2328 Fax: (864) 369-1149

Customer: _____

(Bill To): _____

BILL TO:
Cascade Orthopedic Supply
 2638 Aztec Drive • Chico, CA 95928

Contact: _____

Phone: _____

Transfemoral (AK) Test Socket by Measurement

Date: _____ Date Required: _____

P.O. Number: _____

Ship To: _____

Ground Next Day Air 2 Day
 3 Day Other _____

Patient Name: _____ Sex: _____ Height: _____ Weight: _____ Age: _____

Brim Style _____ **Side** _____ **Spacing** _____ **Other** _____
 50 mm(Std) / _____

MEASURE IN MILLIMETERS, PLEASE

Measurements Taken By: _____

Part numbers are provided in case your PO requires these specifics internally or you are ordering through a distributor.

Options

Reduction % _____

Base Part

Carving Only, Standard Size

#STF0006

Carving Only, Oversize

#STF0006XL

Tests Socket (send carving? Y / N)

Test Socket PETG

#STF0010

Test Socket PETG XL*

#STF0010XL

Test Socket Orfitrans Stiff

#STF0110

Test Socket Orfitrans Stiff XL*

#STF0110XL

*Choose XL base part # if residual limb is over 635mm (25") at the 0 circumference or over 483mm (19") in length.

Distal End Shape

Round



Conical



Flat



Add On Part

Pull with lock space

add #STF0029**

Lock part # _____

Supply Lock Y / N

Set up for use of suction or expulsion valve

add #STF0022**

Valve part # _____

Supply Valve Y / N

Set up for use of distal adapter

add #STF0030**

Adapter part # _____

Supply Adapter Y / N


**Does not include supplying component - call us or check our catalog for specific component part #s.

Supply Socks: Y or N

Qty _____ Ply _____

Qty _____ Ply _____

Qty _____ Ply _____

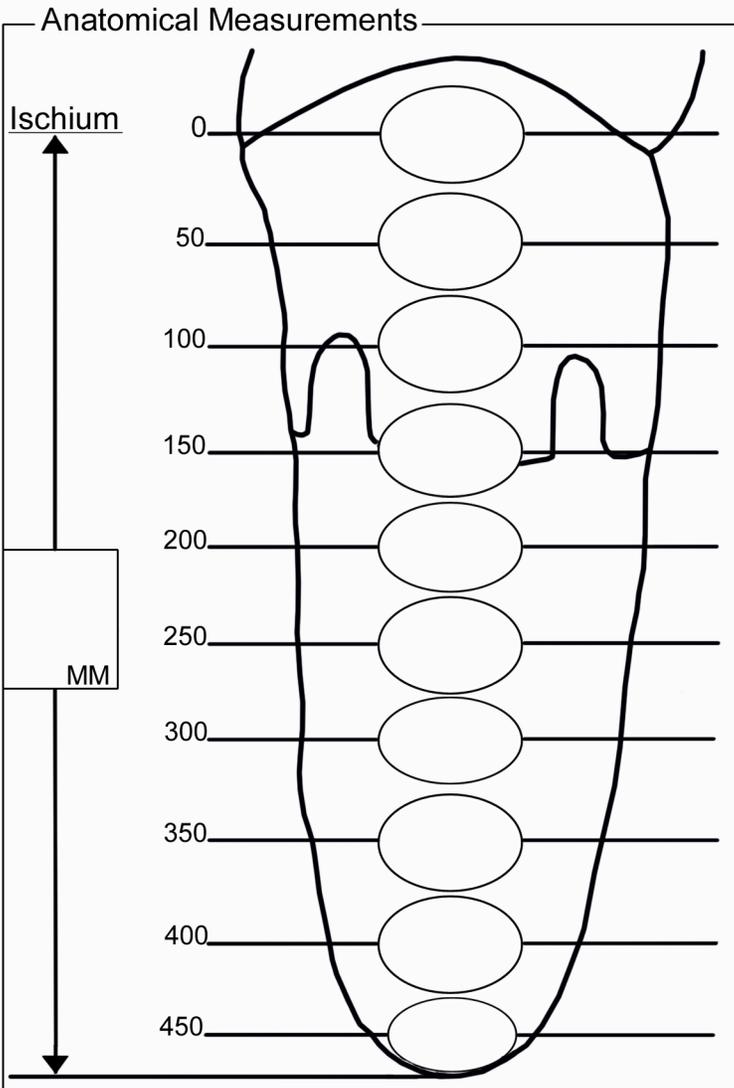

Click HERE to submit form