

GOMEZ ORTHOTIC SYSTEMS
SPINAL MEASUREMENT FORM

DATE _____ TAKEN BY _____ ORDER # _____

SHIP VIA _____ REQUESTED DUE DATE _____ PO # _____

ACCOUNT _____ PHONE _____ CONTACT _____

SHIP TO _____

ADDRESS _____ STATE _____ ZIP _____

PATIENT INFORMATION

NAME _____ PHYSICIAN _____

MALE FEMALE DOB _____ AGE _____ HEIGHT _____ WEIGHT _____

DIAGNOSIS _____ PRESCRIPTION _____

CONTACT _____ PHONE _____


FLEXIBILITY 0-20% 20%-40% 40%-60% 60%-80% 80%-100%


BRACE TYPE CTLSO CTO TLSO LSO POSTERIOR SHELL

OPENING SINGLE ANTERIOR POSTERIOR TONGUE BI-VALVE

MATERIAL _____ THICKNESS _____ FOAM _____ TRANSFER PAPER _____

NOTES _____

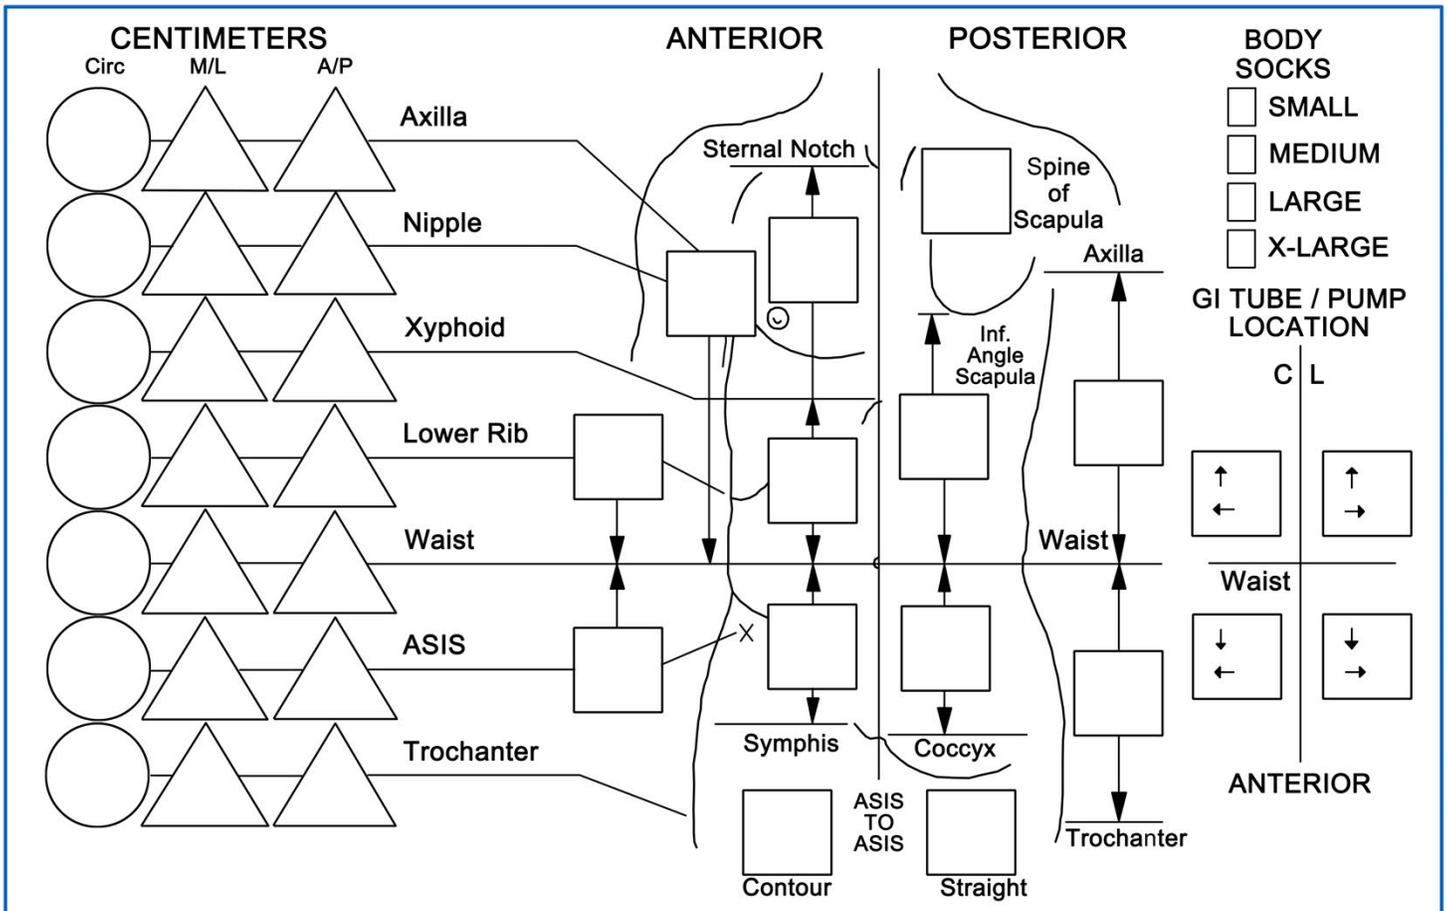

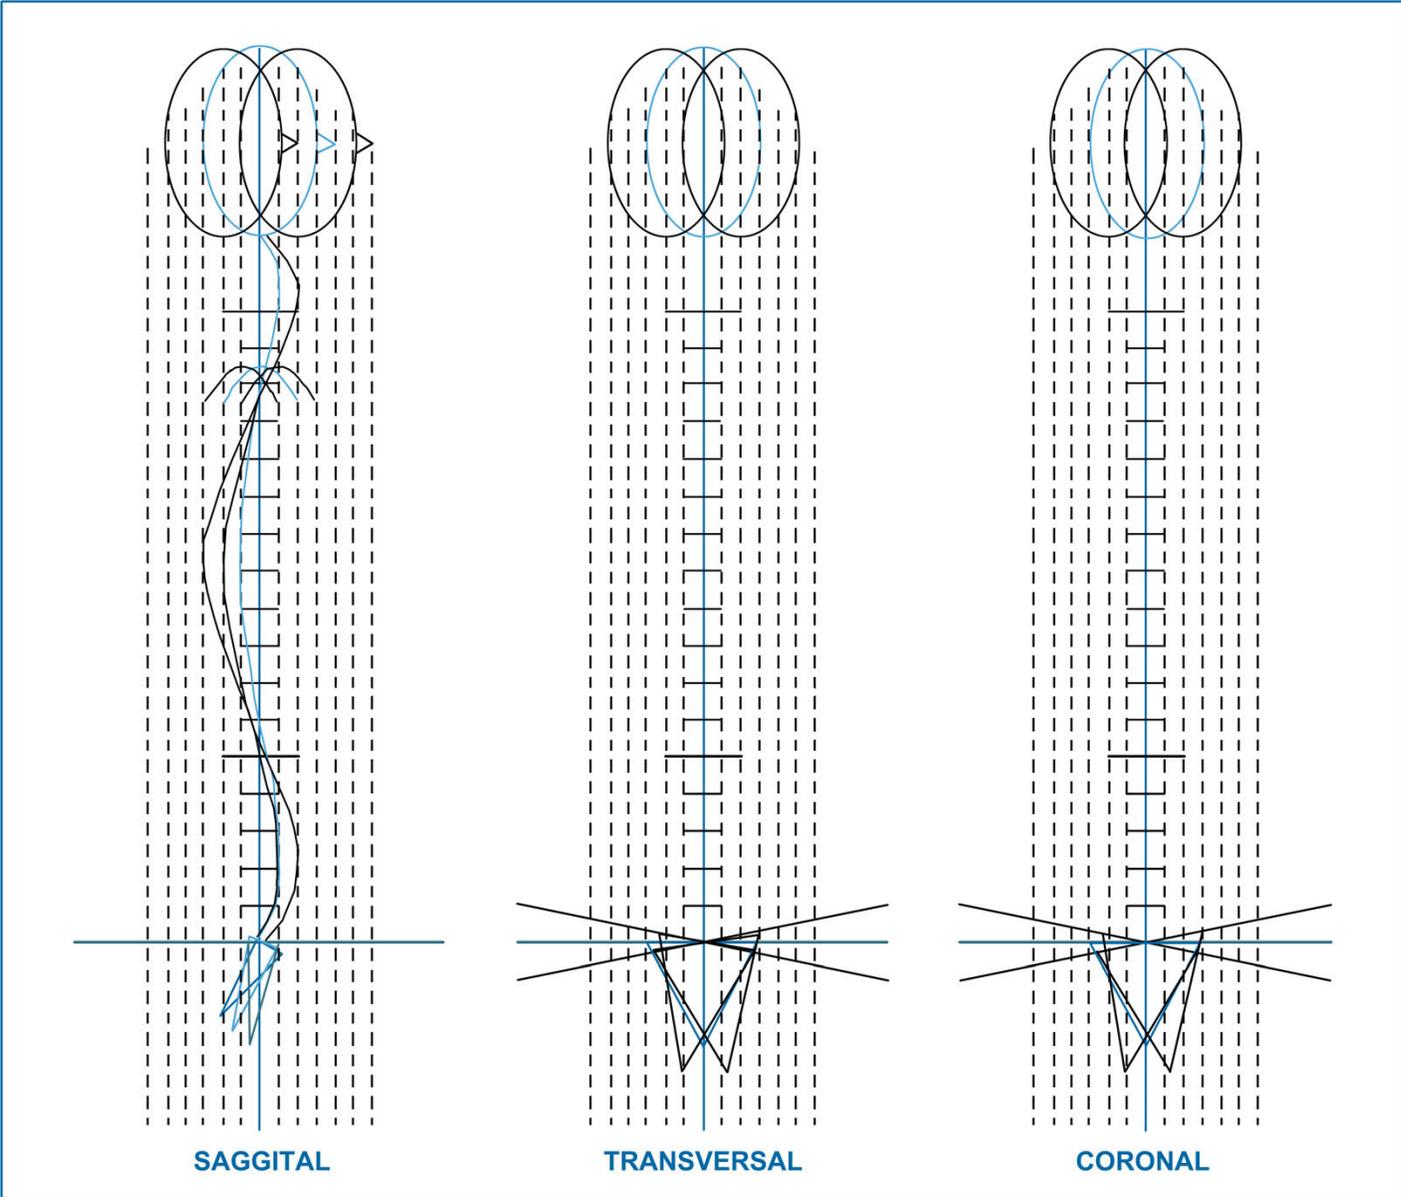

SAGGITAL

TRANSVERSAL

CORONAL

COMMENTS: _____



Gomez Orthotic Systems
 Jose Miguel Gomez T., MD, LO
 jmgomezmd@gorthoticsystems.com
 Mobile: (713) 870-0662
 Fax: (727) 289-2382



Friddle's Orthopedic Appliances, Inc.
 Rachel Friddle-Johnson, CPO
 rfjohnson@friddles.com
 Phone: (800) 528-9339
 Fax (800) 982-3646