

BUNNELL# 6A-MINI **SIZE 1**

WENIGER

915 Industrial Way, San Jacinto, CA 92582 USA

PH: (951) 654-2333 FAX: (951) 654-2331

www.BunnellSplints.com

Authorized Representative:

Medica Surgical Innovations Limited

Moorgate Street

Blackburn BB2 4PB

Lancs UK

CAUTION: Federal Law restricts this device to sale by or on the order of a physician

Printed on Recycled Paper



Single patient use



BUNNELL #6A-MINI

SIZE 1

- >Modified Safety Pin Splint to extend D.I.P joint.
- >Aangepaste Safety Pin Spalk met veer voor vinger extensie.
- >Attelle d'extension modifiée pour un doigt et munie d'une épingle de sûreté.
- >Abgewandelter Sicherheitdnadel Splint zur Streckung eines Langfingers.
- >Stecca a spilla di sicurezza modificata per l'estensione di un dito.
- >Entablillado modificado con clavija de seguridad para extender un dedo.

BUNNELL# 6A-MINI **SIZE 1**

WENIGER

915 Industrial Way, San Jacinto, CA 92582 USA

PH: (951) 654-2333 FAX: (951) 654-2331

www.BunnellSplints.com

Authorized Representative:

Medica Surgical Innovations Limited

Moorgate Street

Blackburn BB2 4PB

Lancs UK

CAUTION: Federal Law restricts this device to sale by or on the order of a physician

Printed on Recycled Paper



Single patient use



BUNNELL #6A-MINI

SIZE 1

- >Modified Safety Pin Splint to extend D.I.P joint.
- >Aangepaste Safety Pin Spalk met veer voor vinger extensie.
- >Attelle d'extension modifiée pour un doigt et munie d'une épingle de sûreté.
- >Abgewandelter Sicherheitdnadel Splint zur Streckung eines Langfingers.
- >Stecca a spilla di sicurezza modificata per l'estensione di un dito.
- >Entablillado modificado con clavija de seguridad para extender un dedo.

BUNNELL# 6A-MINI **SIZE 1**

WENIGER

915 Industrial Way, San Jacinto, CA 92582 USA

PH: (951) 654-2333 FAX: (951) 654-2331

www.BunnellSplints.com

Authorized Representative:

Medica Surgical Innovations Limited

Moorgate Street

Blackburn BB2 4PB

Lancs UK

CAUTION: Federal Law restricts this device to sale by or on the order of a physician

Printed on Recycled Paper



Single patient use



BUNNELL #6A-MINI

SIZE 1

- >Modified Safety Pin Splint to extend D.I.P joint.
- >Aangepaste Safety Pin Spalk met veer voor vinger extensie.
- >Attelle d'extension modifiée pour un doigt et munie d'une épingle de sûreté.
- >Abgewandelter Sicherheitdnadel Splint zur Streckung eines Langfingers.
- >Stecca a spilla di sicurezza modificata per l'estensione di un dito.
- >Entablillado modificado con clavija de seguridad para extender un dedo.

BUNNELL# 6A-MINI **SIZE 1**

WENIGER

915 Industrial Way, San Jacinto, CA 92582 USA

PH: (951) 654-2333 FAX: (951) 654-2331

www.BunnellSplints.com

Authorized Representative:

Medica Surgical Innovations Limited

Moorgate Street

Blackburn BB2 4PB

Lancs UK

CAUTION: Federal Law restricts this device to sale by or on the order of a physician

Printed on Recycled Paper



Single patient use




BUNNELL #6A-MINI

SIZE 1


- >Modified Safety Pin Splint to extend D.I.P joint.
- >Aangepaste Safety Pin Spalk met veer voor vinger extensie.
- >Attelle d'extension modifiée pour un doigt et munie d'une épingle de sûreté.
- >Abgewandelter Sicherheitdnadel Splint zur Streckung eines Langfingers.
- >Stecca a spilla di sicurezza modificata per l'estensione di un dito.
- >Entablillado modificado con clavija de seguridad para extender un dedo.

INSTRUCTIONS #6A MINI Modified Safety Pin Splint
 Dynamic Coiled Spring.
 Open strap. Place finger into splint with curved finger band on bottom and in front of D.I.P. joint.
 Align coiled spring with D.I.P. joint. Position pad on strap (hook and loop compatible), pass strap over top of finger, under lateral wire, and back on top of finger. Secure to loop. Adjust as needed.
 Evaluate fit, function and instruct patient on use.
 Lateral wires and finger bands can be carefully reshaped to improve fit and function. Remove from patient to modify.
 Clean with mild soap and damp towel. Air dry completely before reapplying.
 Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

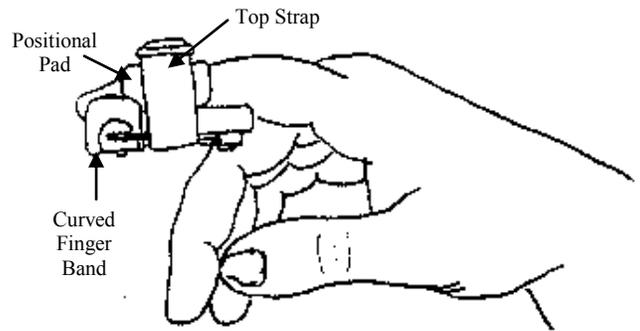


Bunnell #6A MINI Modified Safety Pin Splint to straighten D.I.P. joint

INSTRUCTIONS #6A MINI Modified Safety Pin Splint
 Dynamic Coiled Spring.
 Open strap. Place finger into splint with curved finger band on bottom and in front of D.I.P. joint.
 Align coiled spring with D.I.P. joint. Position pad on strap (hook and loop compatible), pass strap over top of finger, under lateral wire, and back on top of finger. Secure to loop. Adjust as needed.
 Evaluate fit, function and instruct patient on use.
 Lateral wires and finger bands can be carefully reshaped to improve fit and function. Remove from patient to modify.
 Clean with mild soap and damp towel. Air dry completely before reapplying.
 Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

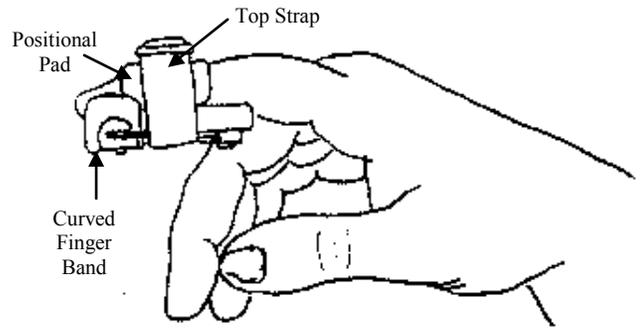


Bunnell #6A MINI Modified Safety Pin Splint to straighten D.I.P. joint

INSTRUCTIONS #6A MINI Modified Safety Pin Splint
 Dynamic Coiled Spring.
 Open strap. Place finger into splint with curved finger band on bottom and in front of D.I.P. joint.
 Align coiled spring with D.I.P. joint. Position pad on strap (hook and loop compatible), pass strap over top of finger, under lateral wire, and back on top of finger. Secure to loop. Adjust as needed.
 Evaluate fit, function and instruct patient on use.
 Lateral wires and finger bands can be carefully reshaped to improve fit and function. Remove from patient to modify.
 Clean with mild soap and damp towel. Air dry completely before reapplying.
 Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

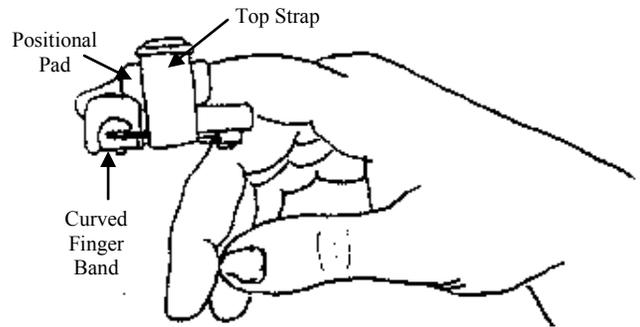

Bunnell #6A MINI Modified Safety Pin Splint to straighten D.I.P. joint

INSTRUCTIONS #6A MINI Modified Safety Pin Splint
 Dynamic Coiled Spring.
 Open strap. Place finger into splint with curved finger band on bottom and in front of D.I.P. joint.
 Align coiled spring with D.I.P. joint. Position pad on strap (hook and loop compatible), pass strap over top of finger, under lateral wire, and back on top of finger. Secure to loop. Adjust as needed.
 Evaluate fit, function and instruct patient on use.
 Lateral wires and finger bands can be carefully reshaped to improve fit and function. Remove from patient to modify.
 Clean with mild soap and damp towel. Air dry completely before reapplying.
 Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

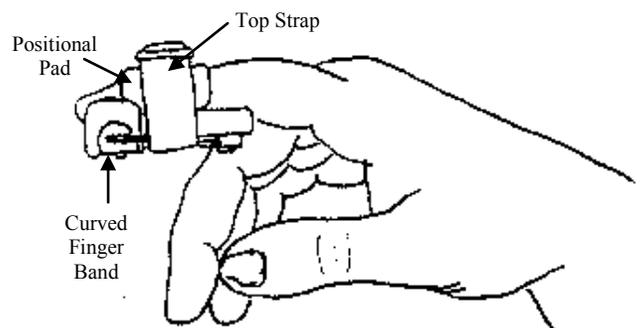

Bunnell #6A MINI Modified Safety Pin Splint to straighten D.I.P. joint